

iCube II

Setup instructions


iCube II is compatible with all Era™ and North platform wireless hearing instruments and can be used for regular fittings, as well as Flex:trial™

Here are the steps to configure the iCube II in Unitron TrueFit™ software:

Step 1

Enable iCube II for fitting

Go to [Options > Preferences > Fitting Device > iCube](#) and check the box [Enable iCube II for fitting](#) for fitting.

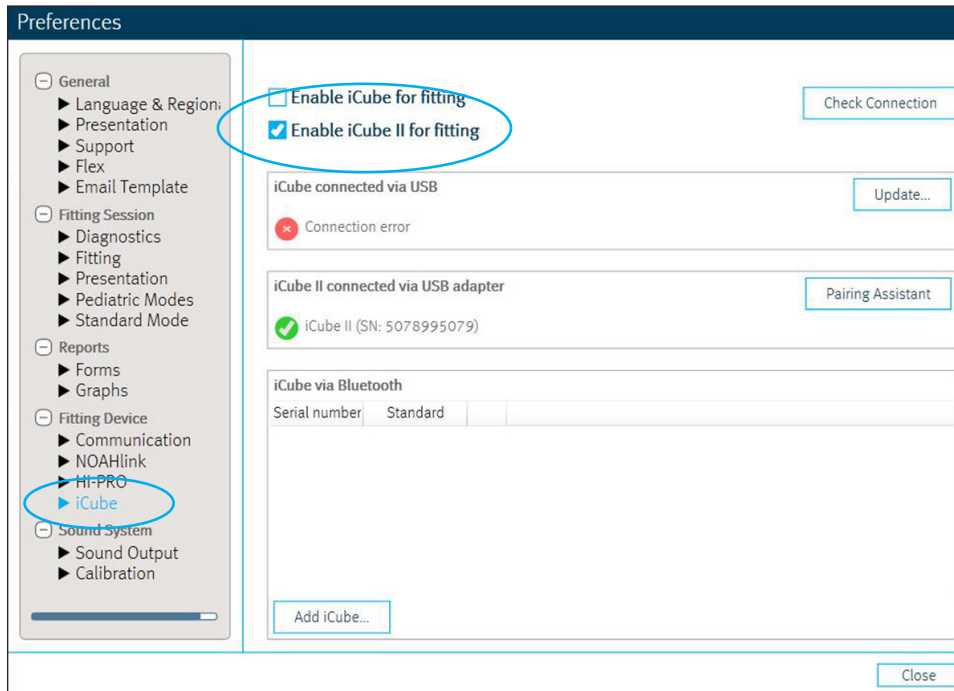

Step 2

Pairing

The iCube II can be paired in the software in [three different ways](#):

a. **Using a wired connection:**

Go to [iCube II connected via USB](#) and follow the steps (same steps as with previous iCube).

b. **Using the Bluetooth adapter that comes with the new iCube II:**

The adapter has to be connected to the USB port of the computer.



Verify that iCube II is turned on, press and hold the pairing button (< >) on the side until the three LED lights flash.

Then, click on the [Pairing Assistant](#) button and follow the instructions on the screen.

c. **Using iCube II via Bluetooth:**


Press and hold the pairing button (< >) on the side until the three LED lights flash to set the iCube II on pairing and follow the 4 steps on the screen.



Step 3

Check the connection


Click on the [Check Connection](#) button. A green check mark will appear next to the iCube II.

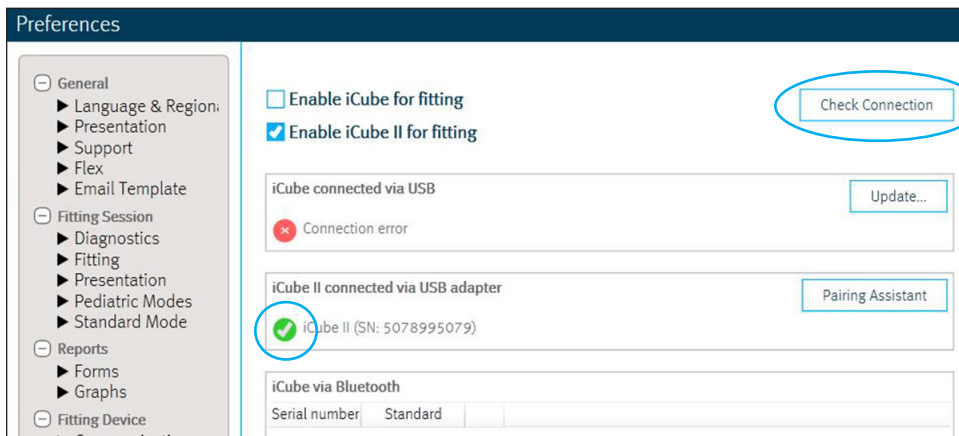

Step 4

End setup

The final step is to go to [Instruments > Selection](#) and select the iCube II as your programming interface.

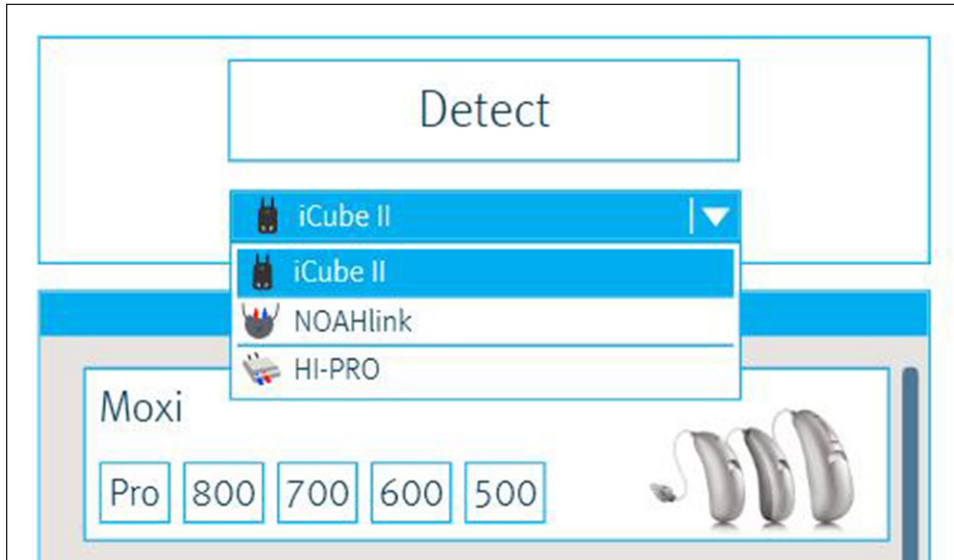

Previous wireless products, like Passport™ and Latitude™ will require the original iCube I for wireless programming, or a wired connection via HiPro or NoahLink.